

10500410

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)


(19) World Intellectual Property Organization
International Bureau(43) International Publication Date
17 July 2003 (17.07.2003)

PCT

(10) International Publication Number
WO 03/058583 A2

- (51) International Patent Classification⁷: **G09B 23/00**
- (21) International Application Number: **PCT/GB02/05844**
- (22) International Filing Date:
20 December 2002 (20.12.2002)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
0200325.9 8 January 2002 (08.01.2002) GB
0213981.4 18 June 2002 (18.06.2002) GB
- (71) Applicant (*for all designated States except US*):
KEYMED (MEDICAL & INDUSTRIAL EQUIPMENT) LTD [GB/GB]; KeyMed House, Stock Road, Southend-on-Sea, Essex SS2 5QH (GB).
- (72) Inventor; and
- (75) Inventor/Applicant (*for US only*): **WALLAKER, Daniel**, [GB/GB]; 94 New Road, Great Wakering, Essex SS3 0AS (GB).
- (74) Agents: **DRAPER, Martyn, John et al.**; **BOULT WADE TENNANT**, Verulam Gardens, 70 Gray's Inn Road, LONDON WC1X 8BT (GB).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).
- Declaration under Rule 4.17:**
— *of inventorship (Rule 4.17(iv)) for US only*
- Published:**
— *without international search report and to be republished upon receipt of that report*
- For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

(54) Title: A DUMMY MEDICAL INSTRUMENT FOR USE IN A SIMULATOR

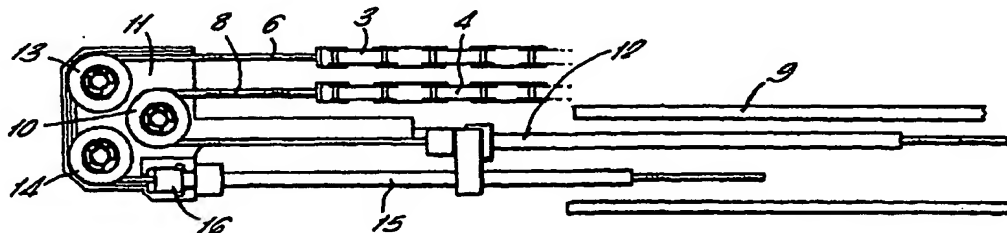

(57) Abstract: A dummy medical instrument for connection to a force feedback mechanism. The dummy medical instrument having a number of cables 5, 8 extending around control knobs 1, 2. In a real instrument corresponding to the dummy instrument, the cables would extend to the tip of the instrument to allow controlled flexing of the tip of the instrument. In the dummy medical instrument, the same cables are routed down the umbilical of the instrument for connection to force feedback motors simulating the forces felt on the tip of the instrument.

WO 03/058583 A2

... AVAILABLE COPY

A DUMMY MEDICAL INSTRUMENT
FOR USE IN A SIMULATOR

5 The present invention relates to a dummy medical instrument for use in a simulator.

10 One type of simulator to which the present invention is applicable is that disclosed in GB A 2252656. This simulator simulates the operation of an endoscopic process. A dummy endoscope is insertable into a fixture which is provided with a sensor mechanism to sense the longitudinal and rotational movement of the dummy endoscope. This information is fed to a controller which generates force feedback information based on virtual model data held in the computer memory. The force feedback applied to the dummy endoscope is synchronised with a visual representation of the procedure so as to provide a realistic simulation providing a useful training tool to endoscope users.

20 With an instrument such as an endoscope, the tip of the endoscope is manipulated by angulation control in the form of one or more control knobs on the handle of the endoscope which are linked to cables which extend down the insertion tube of the endoscope. Turning of the control knobs produces a corresponding movement of the cable and hence the tip. An endoscope can have two control knobs one of which controls the left/right movement of the tip and the other of which controls the up/down movement of the tip.

30 According to the present invention there is provided a dummy medical instrument for use in a simulator, the instrument comprising a control body with user manipulatable angulation control, an insertion tube and an umbilical extending from the

-2-

control body, wherein in a real instrument
corresponding to the one being simulated, at least one
angulation cable would extend from the user
manipulatable controls to the tip of the insertion
5 tube such that movement of the angulation control
changes the angulation of the tip, and wherein in the
dummy medical instrument the angulation cable extends
from the user manipulatable angulation control and
down the umbilical to a device for controlling the
10 resistance to movement of the cable to provide force
feedback simulating the force which would be felt at
the angulation control of a real instrument.

With this arrangement, force feedback is provided
15 to the angulation control whilst using the angulation
control and cable of the real instrument (albeit with
the cable being routed differently). This not only
provides a realistic feel, but also has the advantage
that fewer original components need to be designed for
20 the dummy instrument which also has benefits in terms
of supplying users with replacement parts.

In the real instrument, the cables extend away
from the angulation control in the direction along the
25 insertion tube. One option for the present invention
is to reroute the cables completely so that they
extend away from the angulation control in the
direction of the umbilical. However, the current
preference is for the cable to extend away from the
30 angulation control towards the insertion tube as in
the real body, and to be turned back on itself to
reroute it along the umbilical. There is limited
space available in the control body, and this approach
provides the best way of routing the cables without
35 interfering with other components in the control body.

Within the constraints of the normal instrument,

-3-

there is very little space available to turn the cable back on itself so that it is difficult to avoid generating undesirable friction which can distort the force feedback and cause premature wear of the cable.

5 Therefore, preferably the cable extends from the control body and around a pulley where it is turned through substantially 180° before being routed down the umbilical.

10 The use of the pulley eliminates sliding friction on the cable where it is turned back on itself. This provides not only smoother operation of the force feedback system, but also reduces the wear on the cable.

15 Preferably, the angulation cable is a co-axial cable in which a central wire is moveable within a sleeve. The sleeve is preferably removed for the portion of the cable surrounding the pulley, such that
20 the wire engages directly with the pulley.

When more than one angulation cable is used, each cable should be provided with its own pulley system. In one particularly advantageous arrangement, a first
25 cable is wrapped around a single pulley, while a second cable is wrapped around a pair of pulleys which are spaced apart so that the second cable forms a loop outside of the loop formed by the first cable.

30 In order to retain the cable on the pulley, the or each pulley preferably has a convex periphery, and at least a part of the periphery of the pulley is provided adjacent to the facing wall of a pulley housing.

35 An example of a dummy medical instrument constructed in accordance with the present invention

-4-

will now be described with reference to the accompanying drawings, in which:

Fig. 1 is a plan view of the angulation system;
5 and

Fig. 2 is a schematic perspective view showing the arrangement of pulleys, cables and angulation control.

10 The particular medical instrument being described here is an endoscope. However, it may be any medical instrument where cables which are normally manipulated to move a part of the instrument have to be rerouted so that force feedback can be applied to the cable.

15 The described arrangement is adapted from a conventional endoscope control body. Both of the real and dummy endoscopes have an insertion portion leading from the control body ending at the endoscope tip. In
20 the real instrument, this tip is manipulated to steer it through the colon. An umbilical is provided in both the real and dummy endoscopes leading from the control body to feed various cables to the control body.

25 The control body is provided with a pair of co-axial rotatable knobs 1,2 as shown in Fig. 2. The outer knob 1, in this case, would, in a normal endoscope, be rotated to move the tip in an up/down
30 direction, while the inner knob 2 would move the tip in a left/right direction orthogonal to the up/down direction. These described directions are only notional directions as, in use, the endoscope may be used in any orientation. Wrapped around each pulley
35 is a wire chain drive 3,4 to each of which a cable is attached. In the illustrated example there are four cables which, for convenience, are denoted up cable 5,

-5-

down cable 6, left cable 7 and right cable 8.

5 In a normal instrument, these cables 5,6,7,8 would extend all the way to the tip of the endoscope to provide the tip movement referred to above upon rotation of the knobs 1,2.

10 In the dummy instrument, these cables must be rerouted along the umbilical of the instrument which directs them to an angulation feedback controller. In the angulation feedback controller, the up/down cables 5,6 are connected to opposite sides of a force feedback motor and the left/right cable 7,8 are connected to a similar motor.

15
20 Rotation of the knobs 1,2 is detected and a system controller interprets this information together with information on the longitudinal and rotational positions of the tip of the endoscope. Using data representing a simulated model of a colon, software detects when the simulated tip of the endoscope comes into contact with the simulated colon wall. At this time, the controller sends a force feedback signal to the two feedback motors which hence provides a
25 resistance to the movement of the cables 5-8 which is felt at the knobs 1,2 as a resistance to turning.

30 In order to route each cable into the umbilical 9, the arrangement shown in Fig. 1 and 2 is employed. Fig. 1 shows the rerouting of two of the cables, namely the down cable 6 and the right cable 8. A similar arrangement is provided on the opposite side of the control body as shown in Fig. 2. However, as this has the same construction and operation as the
35 down/right configuration shown in Fig. 1, only this configuration is described in detail. The right cable 8 is connected to the chain 4 that surrounds the inner

-6-

knob 2. This cable then extends around a first pulley
10 rotatably mounted on a housing 11 within the
control body. The pulley 10 turns the right cable
through 180°. A sheath 12 is connected to the housing
5 11. The cable 8 enters the sheath 12 at this point
and is guided within this sheath into the umbilical
which leads it to the feedback motor.

The down cable 6 passes in a loop outside the
10 right cable 8 around a pair of spaced pulleys 13,14
rotatably mounted on the housing 11. The down cable 6
enters a sheath 15 attached to the housing 11 at
connector 16 and is also guided into the umbilical to
the other force feedback motor as described with
15 reference to the right cable.

20

25

30

35

-7-


CLAIMS

1. A dummy medical instrument for use in a simulator, the instrument comprising a control body with user manipulatable angulation control, an insertion tube and an umbilical extending from the control body, wherein in a real instrument corresponding to the one being simulated, at least one angulation cable would extend from the user manipulatable controls to the tip of the insertion tube such that movement of the angulation control changes the angulation of the tip, and wherein in the dummy medical instrument the angulation cable extends from the user manipulatable angulation control, and down the umbilical to a device for controlling the resistance to movement of the cable to provide force feedback simulating the force which would be felt at the angulation control of a real instrument.
2. An instrument according to claim 1, wherein the cable extends from the control body and around a pulley where it is turned through substantially 180° before being routed down the umbilical.
3. An instrument according to claims 1 and 2, wherein the angulation cable is a co-axial cable in which a central wire is moveable within a sleeve.
4. An instrument according to claim 3, wherein the sleeve is removed for the portion of the cable surrounding the pulley, such that the wire engages directly with the pulley.
5. An instrument according to any one of the preceding claims, wherein more than one cable is provided.

-8-

6. An instrument according to claim 2 and claim 5, wherein each cable has its own pulley system.
7. An instrument according to claim 6, wherein a
5 first cable is wrapped around a single pulley, while a second cable is wrapped around a pair of pulleys which are spaced apart so that the second cable forms a loop outside of the loop formed by the first cable.
- 10 8. An instrument according to claim 2 or any one of claims 3, 6 or 7 when dependent on claim 2, wherein the or each pulley preferably has a convex periphery, and at least a part of the periphery of the pulley is provided adjacent to the facing wall of a pulley
15 housing.

2/2

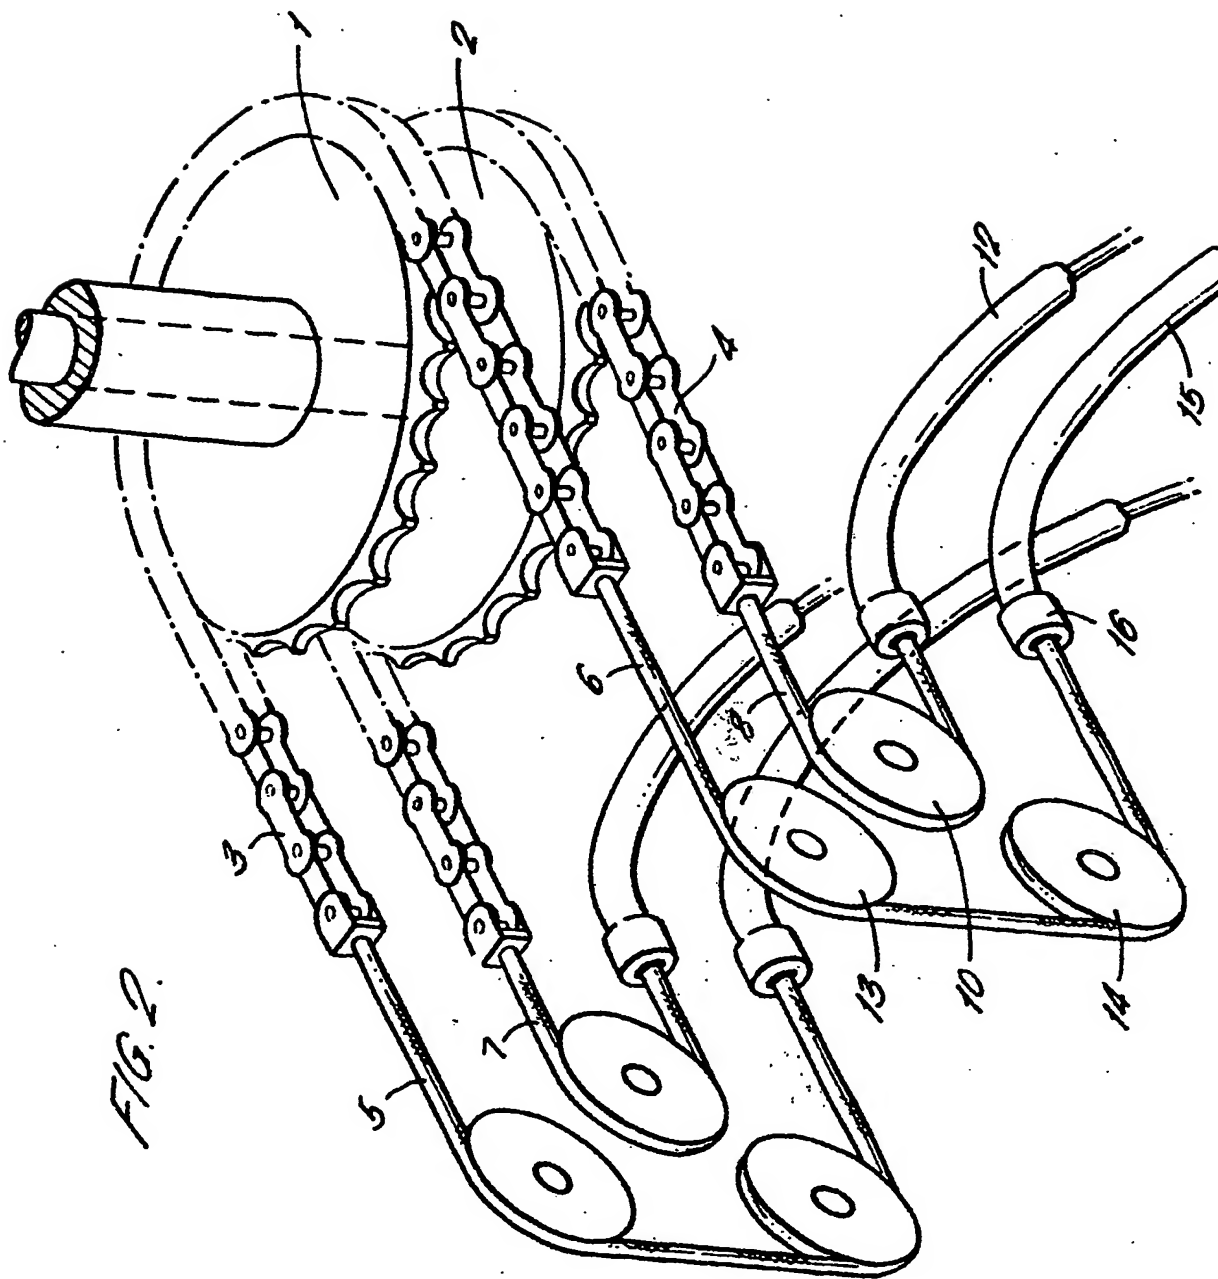

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
17 July 2003 (17.07.2003)

PCT

(10) International Publication Number
WO 03/058583 A3

(51) International Patent Classification⁷: **G09B 23/28**

(21) International Application Number: PCT/GB02/05844

(22) International Filing Date:
20 December 2002 (20.12.2002)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
0200325.9 8 January 2002 (08.01.2002) GB
0213981.4 18 June 2002 (18.06.2002) GB

(71) Applicant (*for all designated States except US*):
**KEYMED (MEDICAL & INDUSTRIAL EQUIP-
MENT) LTD** [GB/GB]; KeyMed House, Stock Road,
Southend-on-Sea, Essex SS2 5QH (GB).

(72) Inventor; and

(75) Inventor/Applicant (*for US only*): **WALLAKER, Daniel**,
[GB/GB]; 94 New Road, Great Wakering, Essex SS3 0AS
(GB).

(74) Agents: **DRAPER, Martyn, John et al.**; **BOULT WADE
TENNANT**, Verulam Gardens, 70 Gray's Inn Road, LON-
DON WC1X 8BT (GB).

(81) Designated States (*national*): AE, AG, AL, AM, AT, AU,
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,

CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH,
GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC,
LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW,
MX, MZ, NO, NZ, OM, PH, PL, PT, RO, RU, SC, SD, SE,
SG, SK, SL, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ,
VC, VN, YU, ZA, ZM, ZW.

(84) Designated States (*regional*): ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE,
ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, SK,
TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GQ,
GW, ML, MR, NE, SN, TD, TG).


Declaration under Rule 4.17:
— *of inventorship (Rule 4.17(iv)) for US only*

Published:
— *with international search report*
— *before the expiration of the time limit for amending the
claims and to be republished in the event of receipt of
amendments*

(88) Date of publication of the international search report:
18 September 2003

*For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.*

(54) Title: A DUMMY MEDICAL INSTRUMENT FOR USE IN A SIMULATOR

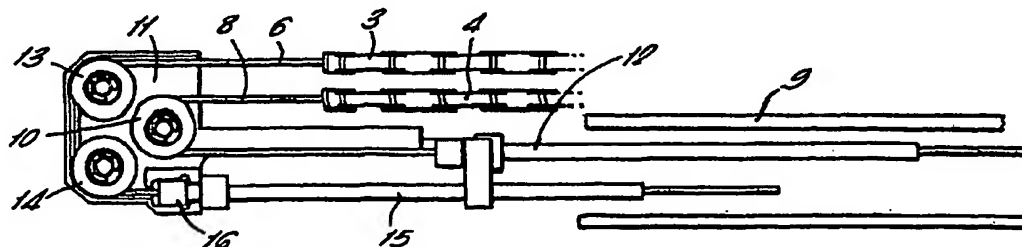

(57) Abstract: A dummy medical instrument for connection to a force feedback mechanism. The dummy medical instrument having a number of cables 5, 8 extending around control knobs 1, 2. In a real instrument corresponding to the dummy instrument, the cables would extend to the tip of the instrument to allow controlled flexing of the tip of the instrument. In the dummy medical instrument, the same cables are routed down the umbilical of the instrument for connection to force feedback motors simulating the forces felt on the tip of the instrument.

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/GB 02/05844

A. CLASSIFICATION OF SUBJECT MATTER
IPC 7 G09B23/28

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G09B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	GB 2 252 656 A (KEYMED) 12 August 1992 (1992-08-12) cited in the application figures 1,2 page 6, line 31 -page 8, line 5 -----	1
A	WO 01 88881 A (BRONSTEIN RAN ;BARKAY DAVID (IL); CHOSACK EDNA (IL); SIMBIONICS LT) 22 November 2001 (2001-11-22) abstract figure 6 page 13, line 15 -page 14, line 11 -----	1

☐ Further documents are listed in the continuation of box C.☒ Patent family members are listed in annex.

* Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *G* document member of the same patent family

Date of the actual completion of the international search

23 July 2003

Date of mailing of the international search report

04/08/2003

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Hanon, D

INTERNATIONAL SEARCH REPORT

International Application No

PCT/GB 02/05844

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
GB 2252656	A	12-08-1992	NONE	
WO 0188881	A	22-11-2001	AU 4872701 A	26-11-2001
			WO 0188881 A2	22-11-2001

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☒ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☐ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.